

# **VERYfinder DETECTION ASSAY**

## **EQUINE (EU)**

Cat. N. PMA11A

### **User Guide**

## 1 - Introduction

The recent scandal related to horse meat sold as bovine put under a spotlight the fact that food industry and consumers, even though the scope is different, share a common interest in the possibility to have a fast and accurate method determining the authenticity of the ingredient used for food preparation.

The food industry often makes use of products, where it is difficult to verify the real content in raw material stated by the manufacturer. This problem translates into economic and commercial risks for the company. On the other side consumers want to be sure the products they eat: deserve the price; don't contain risks for health; are not infringing religious/ethical rules.

DNA testing allows an efficient and sensitive identification of plant and animal derivatives, easily detecting accidental contaminations or potential fraud related to false declaration on the label of the species constituting the food.

Real-Time PCR is the most sensitive method for the detection and quantification of specific DNA sequences of different species. The method combined with an appropriate nucleic acid extraction system allows the analysis of raw materials, semi-finished and finished products as well.

This assay provides the user with a simple and reliable procedure for detecting the presence of the DNA of a specific organisms in food matrices. The assay utilizes the Polymerase Chain Reaction (PCR) to amplify a genetic target typical of the equine (species of interest) according with the official note by the European Union Reference Laboratory for Animal Proteins in feeding stuffs (EURL-AP recommended protocol version 1.0, application and publication day 18.02.2013. <http://eurl.craw.eu/en/187/method-of-reference-and-sops> ).

The validation performed at Generon exploited ION Force DNA Extractor FAST (Cat. N. EXD001) as DNA extraction method from raw and heat treated matrices (20' at 121°C). The Limit of detection (LOD 0.01%) and the Limit of Quantification (LOQ 0.05%) have been calculated based upon a solution concentrated at 2 ng/μl (DNA/DNA) containing equine DNA on a background of DNA from a simulating matrix. These representing the minimum detectable amount of sought species after spiking a simulating matrix. This approach has been used in both raw matrices and heat treated matrices due to the impossibility of having a real standard as each matrix undergoes a different industrial process. Species can moreover be unevenly distributed in the matrix or separated in the homogenization process.

Due to the high sensibility of the test some matrices might cause a background signal, we therefore suggest to operate a DNA quantification after the extraction and to normalize its concentration accordingly to our validation. The plot should then be evaluated using the positive controls provided in the assay. Cut off is strictly dependent from the positive control provided.

## 2 - VERYfinder Equine (EU) Semi-Quantitative Detection Assay

When used along with GENERase Mastermix (Cat. N. ENG001) this Real-Time PCR assay detects a specific DNA sequence in the DNA of equine in less than 1.5 hours. The amplification of the target sequence is measured by the use of a specific fluorescence-labeled probe (FAM).

### 2.1 - Assay Content

	Box 50 reactions		Box 100 reactions	
	N. vials	Volume (μl)	N. vials	Volume (μl)
VERYfinder OLIGO Mix * (OLIGOS and Probe pre-blended mix)	1	625	2	625
Positive Control	1	125	1	125
Negative Control	1	1000	1	1000

*\* reagents are supplied with a 5% of extra volume.*

We suggest to use VERYfinder Equine (EU) Detection Assay along with the following Polymerase Enzyme Ready-to-use mastermix: GENERase Mastermix (Cat. N. ENG001).

### 2.2 - Storage & Expiry information

Expiry date: see date on the packaging, product validity refers to the product kept intact in its original packaging. Protect reagents from light exposure as far as OLIGO Mix reagents are photosensitive. Store frozen.

## 3 – Materials and equipments needed

### 3.1 – Extraction<sup>(1)</sup>

Material/Equipment	Source
Extraction Kit	Generon ION Force DNA extractor FAST (Cat. N. EXD001)
Chemicals: n-esane	Lab Suppliers
Tubes, 50 ml and 15 ml	Lab Suppliers
DNase/RNase Free Water	Lab Suppliers
Vortexer	Lab Suppliers
Benchtop Centrifuge for 50 ml Tubes	Lab Suppliers
Thermal Water Bath or Block	Lab Suppliers
Pipette sets	Lab Suppliers
Pipette tips (Barrier)	Lab Suppliers
Tube rack for 1.5 ml tubes	Lab Suppliers
2.0 and 1.5 ml micro-tubes	Lab Suppliers
Micro centrifuge for 1.5-2.0 ml micro-tubes	Lab Suppliers
DNA Extraction VACUUM BOX + Vacuum pump or Venturi meter	Lab Suppliers

Each step of sample preparation (grinding, transferring, weighing, etc.) must be done according to GLP so that chance of cross-contamination between samples is minimized. It is recommended to use disposable equipment when possible.

If the food samples are not in a powdered or granular form, they should be processed (grinded or blended) before DNA extraction. The majority of DNA extraction methods supports from 20 to 50 mg of starting material. Generon ION Force DNA Extractor FAST (Cat. N. EXD001) allows processing up to 20 grams of starting material in order to maximize sample's lot representation.

Once the sample has been pulverized/homogenized, it can be weighed and the appropriate amount extracted according to DNA extraction method selected. Refer to manufacturer user manual for extraction procedure details.

### 3.3 – Detection via Real-Time PCR

Material/Equipment	Source
Real-Time PCR System <sup>(2)</sup>	Lab Suppliers
VERYfinder Equine (EU) Detection Assay	Generon (Cat. N. PMA11A)
GENERase Mastermix	Generon (Cat. N. ENG001)
Optical Adhesive Seal and Optical reaction plate or Optical Caps and Strips	Lab Suppliers
Micropipette sets	Lab Suppliers

(1) Equipment necessary only when ION Force DNA Extractor FAST (Cat. N. EXD001) is used.

(2) The assay can be used with Biorad CFX and MiniOpticon, Stratagene MxSeries, ABI 7300-7500-Step ONE-StepONE Plus, Light Cycler 480, Eppendorf realplex, Rotor-Gene Q etc. The assay is not compatible with Roche Light Cycler I and II.

## 4 – Real-Time PCR detection

### 4.1 – Reaction setup

- I. Allow the reagents to thaw (GENERase Mastermix, VERYfinder OLIGO MIX, Positive Controls and Negative Control). Vortex tubes when thawed and spin to collect contents at the bottom of the vial.
- II. Mix 625 µl of VERYfinder OLIGO Mix with 875 µl of GENErase Mastermix to prepare VERYfinder Working Mastermix (WMX).
- III. Vortex briefly and spin down in order to homogenize the mix.
- IV. Transfer 30 µl of WMX into each well.
- V. Add 5 µl of Negative Control into wells acting as negative control.
- VI. Add 5 µl of each sample into wells testing the unknown samples.
- VII. Add 5 µl of Positive Control into wells acting as positive control.
- VIII. Close wells and ensure no bubbles are present at the bottom of the wells.

### 4.2 – Instrument setup


With GENErase Mastermix set the following parameters on your thermocycler:

- I. Total Reaction volume: 35 µl
- II. Fluorophores/Quenchers: Target Equine (FAM/BHQ1-NFQ);
- III. Thermal profile:

Step	T (°C)	Duration	Loops
UNG	50	2 min	1
Taq Activation	95	10 min	1
DNA Denaturation	95	15 sec	40
Annealing/Extension + Plate Reading	50	60 sec	

## 5 – Data Interpretation

Results evaluation must be done according to the analysis software recommended by the Real-Time PCR instrument manufacturer. After performing PCR, each individual sample is analyzed through the instrument software to produce a C<sub>q</sub> value (quantification cycle) for each reporter dye. These values are used to determine the presence (Qualitative Test) of target into the sample. See below an example of the graphics obtained for a positive (Fig. A) control for the target amplification (blue line).

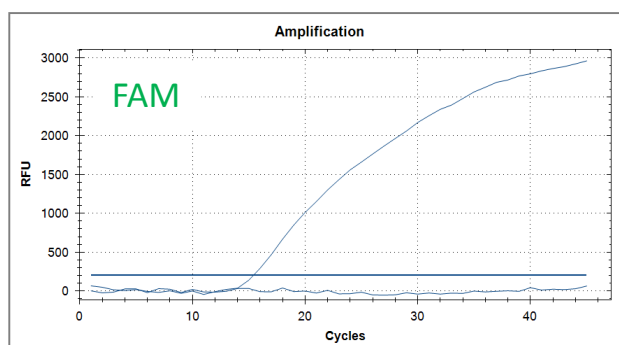

After setting the baseline, the analysis outcome should be evaluated following the indications below.

If the following conditions are met:

TEST	Equine EU (FAM )
Positive Control	+
Negative Control	-

Then the possible results for any sample are:

TEST	Equine EU (FAM )
Positive Sample	+
Negative Sample	-

In case of inhibition DNA isolation and purification for the sample need to be improved or you may need to dilute your sample before performing a new test. Refer to the Troubleshooting paragraph (section 6) for further suggestions.

## 6 – Troubleshooting

- I. Concomitant no target or IAC amplification or amplification plots grossly abnormal. Possible causes and corrective actions:
  - An excess of DNA in the target might inhibit the reaction may be affected due to an excess of DNA and/or PCR inhibitors. Test samples diluted 1:10 and 1:100. Please, use DNase/RNase Free Water to prepare dilutions.
  - Inadequate sealing of optical caps/film caused sample evaporation. Redo the analysis using proper tools and proper optical caps/film to secure perfect sealing.
  - Did not use the proper consumables. Redo the analysis and use only optical grade 96-well plates and optical adhesive seal or optical 8-well strips and caps.
  - Samples were not properly prepared. Remake the sample DNA preps. Ensure that the DNA extraction method is properly performed.
- II. Positive Control reactions failed to amplify, but other reactions appear correct (e.g. the IAC is amplified):
  - Positive Controls DNA were not added to the reaction wells. If other reactions look normal, there may be no need to repeat the run.
- III. Negative Control reactions are positive:
  - Contamination of the negative control vial or the VERYfinder PCR mix with VERYfinder-positive DNA. Use more care to prevent contamination while handling assay reagents and setting up assays.

In case support is needed contact Generon at: [support@generon.it](mailto:support@generon.it)

## 7 – Disclaimers

The product is intended for research use only. Generon makes no warranty of any kind, either expressed or implied, except that the materials from which its products are made of standard quality. If any materials are defective, Generon will provide a replacement product. Generon shall not be liable for any damages, including special or consequential damage, or expense arising directly or indirectly from the use of this product. Please do not interchange components between assays of different lot numbers. This assay is designed to be used by laboratory personnel following the common molecular biology precautions.

## Quick Reference Guide

Page 1

Product Line:	VERYfinder
Type:	Qualitative
Storage:	Frozen
Execution time:	about 120 minutes
Expiry date:	see date on the packaging, product validity refers to the product kept intact in its original packaging and constantly under suitable temperature conditions as mentioned above.

### Assay Box Content

	Box 50 reactions		Box 100 reactions	
	N. vials	Volume (µl)	N. vials	Volume (µl)
VERYfinder OLIGO Mix (OLIGOS and Probe pre-blended mix)	1	625	2	625
Positive Control	1	125	1	125
Negative Control	1	1000	1	1000

All reagents are supplied with a 5% of extra volume.

Not Provided Article: GENERase Mastermix (Cat. N. ENG001) or equivalent.

### Reaction Set-Up

Protect reagents from light exposure as far as OLIGO Mix reagents are photosensitive.

Before setting the analysis, we strongly advise to leave the reagents to warm up at room temperature. Vortex briefly OLIGO mix, afterwards spin to collect contents at the bottom of the vials. Spin GENERase Mastermix (Cat. N. ENG001) before opening it.

Prepare VERYfinder WORKING Mastermix by adding 625 µl of VERYfinder OLIGO Mix into each tube prefilled with 875 µl of GENERase Mastermix (Cat. N. ENG001) in order to obtain a single volume of 1500 µl of VERYfinder WORKING Mastermix. Vortex briefly VERYfinder WORKING Mastermix with the aim of homogenizing the mix and excluding MgCl<sub>2</sub> gradient that could impair the results. Spin to collect contents at the bottom of the vial (*Note: label GENERase vials with target name after OLIGO Mix addition*). Vortex briefly Positive Control and samples before proceeding further, spin to collect contents at the bottom of the vial.

Transfer VERYfinder WORKING Mastermix and samples into the plate as follows:

Reagents per well	Volume
Unknown Sample	5 µl
Positive Control	
Negative Control	
VERYfinder WORKING Mastermix	30 µl
Final Volume	35 µl

### Detector Setup

Target	Reporter Dye	Quencher Dye
EQUINE (EU) Target	FAM	BHQ1-NFQ



## Quick Reference Guide

Page 2

### Thermal cycling

Step	T (°C)	Duration	Loops
UNG	50	2 min	1
Taq Activation	95	10 min	1
DNA Denaturation	95	15 sec	40
Annealing/Extension + Plate Reading	50	60 sec	

The thermal profile presented above was optimized for GENERase Mastermix (Cat. N. ENG001).

### Results analysis

If the following conditions are met:

TEST	Equine EU (FAM )
Positive Control	+
Negative Control	-

Then the possible results for any sample are:

TEST	Equine EU (FAM )
Positive Sample	+
Negative Sample	-

In case of inhibition DNA isolation and purification for the sample need to be improved or you may need to dilute your sample before performing a new test. Refer to the Troubleshooting paragraph , section 6 in the User Guide, for further suggestions.

### Warning and Precaution

Please do not interchange components of assays with different lot numbers. This assay is designed to be used by laboratory personnel following the common molecular biology precautions (GLP).

### Disclaimer

Generon s.r.l. guarantees the buyer exclusively concerning the quality of reagents and of the components used to produce the Assay. Generon S.r.l. is not responsible and cannot anyway be considered responsible or jointly responsible for possible damages resulting from the utilization of the product by the user. The user consciously and under his own responsibilities decides for the utilization purposes of the product and uses it the way he considers most suitable in order to reach his goals and/or objectives.

Generon S.r.l. is not responsible for the data resulting from the use of the products, for the utilization that the user independently decides to make of them or for the damages possibly resulting from the disclosure or transmission of the data themselves to third parties under any form or circumstance. This clause is automatically accepted by the user when purchasing the products. The patent for performing PCR is held by Hoffmann/La Roche. Authorization to use PCR can be obtained on licence from Hoffmann-LaRoche. The product, equipment and information included in the assay consists of assembled and reagents. The licence and licence and authorisation for PCR use are not included in the assay. The user is responsible for setting prefixed goals, choosing whether or not to perform the PCR reaction and to apply for register his own licence. The use assay is designed for the services supply, quality control or any other application that is not exclusively an internal company's research and requires a specific licence for PCR use. This PCR use licence to supply a service on food analysis field has to be requested directly from Applied Biosystems". This assay requires the use of Taq Polymerase enzyme.

The product was internally tested by our quality control. Any responsibility is waived if the warranty of quality control does not refer to the specific product. The user is personally responsible for data that he will obtained and/or he will supply to third parties using this assay. Once the sealed package is open the user accepts all the conditions without fail; if the package is still sealed the product can be returned and the user can be refunded.